



High Sensitivity ELISA Kit

[Catalog No] EK280HS

[SIZE] 48T/96T

[INTENDED USE] For the quantitative determination of mouse Interferon gamma (IFN- γ) concentrations in cell culture supernates, serum and plasma.

[INTRODUCTION]

Interferon gamma (IFN- γ) is a dimerized soluble cytokine that is the only member of the type II class of interferons. IFN- γ is produced predominantly by natural killer (NK) and natural killer T (NKT) cells as part of the innate immune response, and by CD4 Th1 and CD8 cytotoxic T lymphocyte (CTL) effector T cells once antigen-specific immunity develops. IFN- γ , or type II interferon, is a cytokine that is critical for innate and adaptive immunity against viral, some bacterial and protozoal infections. IFN- γ is an important activator of macrophages and inducer of Class II major histocompatibility complex (MHC) molecule expression. Aberrant IFN- γ expression is associated with a number of autoinflammatory and autoimmune diseases. The importance of IFN- γ in the immune system stems in part from its ability to inhibit viral replication directly, and most importantly from its immunostimulatory and immunomodulatory effects. The role of IFN- γ as a disease marker has been demonstrated for a number of different pathological situations including infections, autoimmune diseases, transplant rejection, allergy and diabetes.

[PRINCIPLE OF THE ASSAY]

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for mouse IFN- γ has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and IFN- γ present is bound by the immobilized antibody. After washing away any unbound substances, a biotin-linked detect antibody specific for IFN- γ is added to the wells. Following a wash to remove any unbound antibody-biotin reagent, streptavidin-HRP is added. After washing, amplification reagent is added to the wells. Following incubation any unbound substances is removed during a wash step and streptavidin-HRP is added. After washing, substrate solution is added to the wells and color develops in proportion to the amount of IFN- γ bound in the initial step. The color development is stopped and the intensity of the color is measured.

[MATERIALS PROVIDED]

PART	PART #	EK280HS-48	EK280HS-96
Coated Microplate	EK280HSP	48T	96T
Standard	EK280HSS	1vial	2vials
Detect antibody	EK280HSD	1vial	1vial
Standard Diluent	E0260	5ml	5ml
Streptavidin-HRP	E0290	1vial	2vials
Amplification Reagent Concentrate	E0270	1vial	1vial
Amplification Diluent	E0320	12ml	12ml
Assay Buffer (10 \times)	E0310	5ml	5ml
TMB	E0230	6ml	11ml
Stop Solution	E0300	11ml	11ml
Washing Buffer (20 \times)	E0281	50ml	50ml
Adhesive Film	E0200	10	10

Note: Components from reagent kits of different batch numbers must not be used interchangeably.

OTHER SUPPLIES REQUIRED

- 1) Microplate reader capable of measuring absorbance at 450 nm, with correction wavelength set at 570 nm or 630 nm.
- 2) Pipettes and pipette tips.
- 3) 50 μ l to 300 μ l adjustable multichannel micropipette with disposable tips.
- 4) Multichannel micropipette reservoir.
- 5) Beakers, flasks, cylinders necessary for preparation of reagents.
- 6) Deionized or distilled water.
- 7) Polypropylene test tubes for dilution.

[STORAGE]

Store at 2-8°C; refer to the kit label for expiration date.

For opened kits:

Pre-coated microplate: Can be stored at 2-8°C for approximately 1 month (return unused strips to the aluminum foil bag and reseal).

Standard: Can be stored at -20°C for approximately 1 month (discard after single-use reconstitution).

Other components: Can be stored at 2-8°C for approximately 1 month.

[SAMPLE COLLECTION AND STORAGE]

1) **Cell Culture Supernates** - Remove particulates by centrifugation and assay freshly prepared samples immediately or aliquot and store samples at \leq -20°C for later use. Avoid repeated freeze-thaw cycles.

2) **Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 10 minutes at 1,000 \times g. Remove serum and assay freshly prepared samples immediately or aliquot and store samples at \leq -20°C for later use. Avoid repeated freeze-thaw cycles.

3) **Plasma** - Collect plasma using EDTA, citrate or heparin as anticoagulant. Centrifuge at 1,000 \times g within 30 minutes of collection. Assay freshly prepared samples immediately or aliquot and store samples at \leq -20°C for later use. Avoid repeated freeze-thaw cycles.

4) Other biological samples might be suitable for use in the assay. Cell culture supernates, serum and plasma were tested with this assay.

Dilution with Assay Buffer may be needed.

Note: Samples containing a visible precipitate must be clarified prior to use in the assay. Do not use grossly hemolyzed or lipemic specimens.

If samples are to be run within 24 hours, they may be stored at 2 to 8°C.

For longer storage, aliquot samples and store frozen at -20°C. Avoid repeated freeze-thaw cycles.

[REAGENT PREPARATION]

Bring all reagents and samples to room temperature before use.

If crystals form in the Buffer Concentrates, warm and gently stir them until completely dissolved.

Washing Buffer (1 \times)

Pour entire contents (50 ml) of the **Washing Buffer (20 \times)** into a clean 1,000 ml graduated cylinder. Bring to final volume of 1,000 ml with pure or deionized water.

Mix gently to avoid foaming.

Transfer to a clean wash bottle and store at 2 to 25°C. Washing Buffer (1 \times) is stable for 30 days.

Assay Buffer (1 \times)

Pour the entire contents (5 ml) of the **Assay Buffer (10 \times)** into a clean 100 ml graduated cylinder. Bring to final volume of 50 ml with distilled water. Mix gently to avoid foaming.

Store at 2 to 8°C. Assay Buffer (1 \times) is stable for 30 days.

Detect Antibody

Mix well prior to making dilutions.

Make a 1: 100 dilution of the concentrated **Detect Antibody** solution with Assay Buffer (1 \times) in a clean plastic tube.

The diluted Detect Antibody should be used within 30 minutes after dilution.

Streptavidin-HRP

Mix well prior to making dilutions.

Make a **1: 100** dilution of the concentrated **Streptavidin-HRP** solution with Assay Buffer (1×) in a clean plastic tube as needed.

The diluted Streptavidin-HRP should be used within 30 minutes after dilution.

Amplification Reagent Concentrate

Mix well prior to making dilutions.

Make a **1: 100** dilution of the concentrated **Amplification Reagent** solution with **Amplification Diluent** in a clean plastic tube as needed.

The diluted Amplification Reagent should be used within 30 minutes after dilution.


Sample Dilution: If your samples have high IFN- γ content, dilute serum/plasma samples with Assay Buffer (1×). For cell culture supernates, dilute with cell culture medium.

Mouse IFN- γ Standard: Reconstitute Mouse IFN- γ Standard by addition of distilled water. Reconstitution volume is stated on the label of the standard vial. Swirl or mix gently to insure complete and homogeneous solubilization (concentration of reconstituted standard = 1,000 pg/ml).

Allow the standard to reconstitute for 10 - 30 minutes. Mix well prior to making dilutions.

Use polypropylene tubes.

- For serum/plasma samples, mixing concentrated Mouse IFN- γ standard (230 μ l) with 230 μ l of Standard Diluent creates the high standard (500 pg/ml). Pipette 230 μ l of Standard Diluent into each tube. Use the high standard to produce a 1:1 dilution series (scheme below). Mix each tube thoroughly before the next transfer. Standard Diluent serves as the zero standard (0 pg/ml).
- For cell culture supernates, mixing concentrated Mouse IFN- γ standard (230 μ l) with 230 μ l of cell culture medium creates the high standard (500 pg/ml). Pipette 230 μ l of cell culture medium into each tube. Use the high standard to produce a 1:1 dilution series. Mix each tube thoroughly before the next transfer. Cell culture medium serves as the zero standard (0 pg/ml).

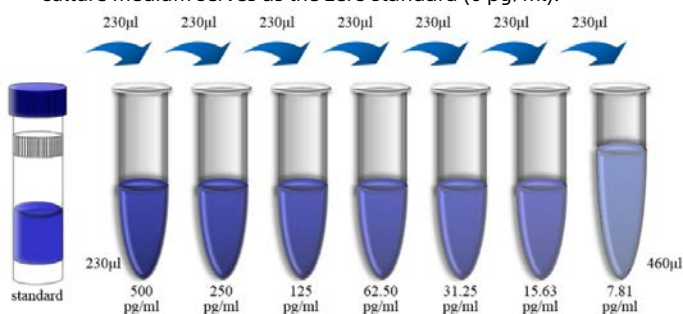

[ASSAY PROCEDURE]

Bring all reagents and samples to room temperature before use.

- 1) Prepare all reagents including microplate, samples, standards and working solution as described in the previous sections.
- 2) Remove excess microplate strips and return them to the foil pouch containing the desiccant pack, and reseal for further use.
- 3) Add 300 μ l Washing Buffer (1×) per well, and allow it for about 30 seconds before aspiration. Soaking is highly recommended to obtain a good test performance. Empty wells and tap microwell strips on absorbent pad or paper towel to remove excess Washing Buffer (1×). Use the microwell strips immediately after washing. **Do not allow wells to dry.**
- 4) Add 100 μ l 2-fold diluted Standard to Standard well. Add 100 μ l

Standard Diluent/ culture medium to Blank well.

5) **Serum/Plasma:** Add 90 μ l Assay Buffer (1×) and 10 μ l sample to the sample well. **Cell culture supernates:** Add 100 μ l cell culture supernates to the sample well. Ensure reagent addition in step 4 and 5 is uninterrupted and completed within 15 minutes.

6) Cover with an Adhesive Film. Incubate at room temperature (25°C±3°C) for 1.5 hours on a microplate shaker set at 300 rpm.

7) Aspirate each well and wash, repeating the process five times for a total six washes. Wash by filling each well with 300 μ l Washing Buffer (1×). Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

8) Add 100 μ l of diluted Detect Antibody to each well. Cover with a new Adhesive Film. Incubate at room temperature (25°C±3°C) for 30 minutes on a microplate shaker set at 300 rpm.

9) Repeat aspiration/wash as in step 7.

10) Add 100 μ l of diluted Streptavidin-HRP to each well. Cover with a new Adhesive Film. Incubate at room temperature (25°C±3°C) for 30 minutes on a microplate shaker set at 300 rpm.

11) Repeat aspiration/wash as in step 7.

12) Add 100 μ l of diluted Amplification Reagent to each well. Cover with a new Adhesive Film. Incubate at room temperature (25°C±3°C) for exactly 15 minutes on a microplate shaker set at 300 rpm.

13) Repeat aspiration/wash as in step 7.

14) Add 100 μ l of diluted Streptavidin-HRP to each well. Cover with a new Adhesive Film. Incubate at room temperature (25°C±3°C) for exactly 15 minutes on a microplate shaker set at 300 rpm.

15) Repeat aspiration/wash as in step 7.

16) Add 100 μ l of Substrate Solution to each well. Incubate for 5 - 30 minutes at room temperature (25°C±3°C). **Protect from light.**


17) Add 100 μ l of Stop Solution to each well. The color will turn yellow. If the color in the well is green or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.

18) Measure the optical density value within 30 minutes by microplate reader set to 450 nm. If wavelength correction is available, set to 570 nm or 630 nm. If wavelength correction is not available, subtract readings at 570 nm or 630 nm from the readings at 450 nm. This subtraction will correct for optical imperfections in the plate. Reading directly at 450 nm without correction may generate higher concentration than true value.

[TYPICAL DATA]

A standard curve must be run within each assay. The following standard curve is provided for demonstration only.

pg/ml	O.D.	Average	Corrected
0.00	0.075	0.076	0.076
7.81	0.086	0.086	0.011
15.63	0.095	0.097	0.021
31.25	0.117	0.117	0.042
62.50	0.182	0.189	0.110
125.00	0.353	0.370	0.286
250.00	0.780	0.777	0.703
500.00	2.434	2.425	2.354

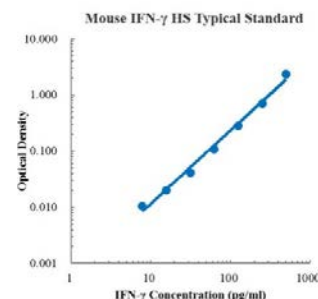

MULTI SCIENCES BIOTECH CO., LTD.

www.multisciences.net

E-mail: service@multisciences.net